



Image Display DICOM Conformance Statement

EasyViz 7.5

Version 1.3

February 21, 2018

Document ID: 2017.03.006

Karos Health Incorporated
7 Father David Bauer Drive
Suite 201
Waterloo, ON
N2L 0A2
Canada
info@karoshealth.com

Karos Health shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance or use of this publication. Karos Health reserves the right to revise this publication and to make changes to its content at any time, without obligation to notify any person or entity of such revisions and changes. This publication may only be used in connection with the promotion, sales, installation and use of Karos Health products.

www.karoshealth.com

Table of Contents

| | |
|---|----|
| 1. Document History..... | 5 |
| 2. Conformance Statement Overview | 6 |
| 3. Introduction..... | 8 |
| 3.1 Audience | 8 |
| 3.2 Remarks | 8 |
| 3.3 Terms and Abbreviations..... | 8 |
| 3.4 References | 9 |
| 4. Networking | 10 |
| 4.1 Implementation Model..... | 10 |
| 4.1.1 Application Data Flow | 10 |
| 4.1.2 Functional Definitions of AE's..... | 11 |
| 4.1.2.1 Functional Definition: Query/Retrieve SCU | 11 |
| 4.1.2.2 Functional Definition: Storage SCU..... | 11 |
| 4.1.2.3 Functional Definition: Storage SCP | 11 |
| 4.1.2.4 Functional Definition: Print Management SCU | 11 |
| 4.1.3 Sequencing of Real World Activities | 11 |
| 4.1.4 AE Specification: Query/Retrieve SCU | 14 |
| 4.1.4.1 SOP Classes | 14 |
| 4.1.4.2 Association Policies | 14 |
| 4.1.4.3 Association Initiation Policy | 14 |
| 4.1.4.4 Association Acceptance Policy..... | 15 |
| 4.1.5 AE Specification: Storage SCU..... | 15 |
| 4.1.5.1 SOP Classes | 15 |
| 4.1.5.2 Association Policies | 17 |
| 4.1.5.3 Association Initiation Policy | 18 |
| 4.1.5.4 Association Acceptance Policy..... | 21 |
| 4.1.6 AE Specification: Storage SCP | 21 |
| 4.1.6.1 SOP Classes | 21 |
| 4.1.6.2 Association Policies | 23 |
| 4.1.6.3 Association Initiation Policy | 24 |
| 4.1.6.4 Association Acceptance Policy..... | 24 |
| 4.1.7 AE Specification: Print Management SCU..... | 39 |
| 4.1.7.1 SOP Classes | 39 |
| 4.1.7.2 Association Policies | 39 |
| 4.1.7.3 Association Initiation Policy | 40 |
| 4.1.7.4 Association Acceptance Policy..... | 40 |
| 4.2 Network Interfaces | 41 |
| 4.2.1 Physical Network Interface | 41 |
| 4.2.2 Additional Protocols | 41 |

| | |
|--|----|
| 4.3 Configuration | 41 |
| 4.3.1 AE Title/Presentation Address Mapping..... | 41 |
| 4.3.1.1 Local AE Titles..... | 41 |
| 4.3.1.2 Remote AE Title/Presentation Address Mapping..... | 41 |
| 4.3.2 Parameters..... | 41 |
| 5. Media Interchange | 42 |
| 5.1 Implementation Model..... | 42 |
| 5.1.1 Application Data Flow Diagram | 42 |
| 5.1.2 Functional Definitions of AE's..... | 43 |
| 5.1.2.1 Functional Definition: Media FSR..... | 43 |
| 5.1.2.2 Functional Definition: Media FSC..... | 43 |
| 5.1.3 Sequencing of Real World Activities | 43 |
| 5.1.4 File Meta Information for Implementation Class and Version | 44 |
| 5.2 AE Specifications..... | 44 |
| 5.2.1 AE Specification: Media FSR | 44 |
| 5.2.1.1 File Meta Information: Media FSR | 44 |
| 5.2.1.2 Real-World Activities | 44 |
| 5.2.2 AE Specification: Media FSC..... | 47 |
| 5.2.2.1 File Meta Information: Media FSC | 47 |
| 5.2.2.2 Real-World Activities | 47 |
| 5.3 Augmented and Private Application Profiles..... | 49 |
| 5.4 Media Configuration | 49 |
| 6. Support of Character Sets..... | 49 |
| 6.1 Overview..... | 49 |
| 6.2 Character Sets..... | 49 |
| 6.3 Character Set Configuration | 49 |
| 7. Security | 49 |
| 7.1 Security Profiles | 49 |
| 7.2 Association Level Security | 50 |
| 7.3 Application Level Security | 50 |
| 8. Annexes | 50 |
| 8.1 IOD Contents..... | 50 |
| 8.1.1 Created SOP Instance(s)..... | 50 |
| 8.1.1.1 Key Object Selection Document IOD..... | 50 |
| 8.1.1.2 Grayscale Softcopy Presentation State IOD | 51 |
| 8.1.1.3 Common Modules | 51 |
| 8.1.1.4 Key Object Selection Document Modules | 53 |
| 8.1.1.5 Grayscale Softcopy Presentation State Modules..... | 54 |
| 8.1.2 Usage of Attributes of Received IOD's..... | 58 |

| | | |
|-------|--|----|
| 8.1.3 | Attribute Mapping | 58 |
| 8.1.4 | Coerced/Modified Fields | 58 |
| 8.2 | Data Dictionary of Private Attributes | 58 |
| 8.3 | Coded Terminology and Templates..... | 58 |
| 8.4 | Grayscale Image Consistency..... | 58 |
| 8.5 | Standard Extended/Specialized/Private SOP Classes | 59 |
| 8.5.1 | MI 3D Softcopy Presentation State Private SOP Class..... | 59 |
| 8.6 | Private Transfer Syntaxes | 59 |

1. Document History

| Revision | Date | Author | Changes |
|----------|------------|---------------------------|---|
| | 2010-07-15 | NHK | Initial draft for EasyViz 3.0.4 Added support for: Multi-frame Grayscale Byte Secondary Image Storage Multi-frame Grayscale Word Secondary Capture Image Storage Multi-Frame True Color Secondary Capture Image Storage |
| | 2011-01-28 | TS | Updated for 3.2 Added VL Image Storage (retired) for Storage SCP. Added JPEG 2000 Lossless Only and JPEG 2000 Lossless and Lossy transfer syntaxes to Storage SCP accepted transfer syntaxes. Updated Implementation Version Name and Implementation Class UID. |
| | 2011-04-19 | JBB | Updated for 3.2. Added Description of GPWL support |
| | 2011-11-29 | TS | Updated for 4.0. No actual changes except document ID, software version and references to other 4.0 documents. |
| | 2013-04-25 | MWN | Updated for 5.0. No actual changes except document ID, software version and references to other 5.0 documents. |
| | 2013-05-07 | MWN | Converted document into new template |
| | 2014-08-05 | MWN | Updated for 6.0. No actual changes except software version and references to other 6.0 documents. |
| | 2015-09-14 | MWN | Updated for 7.0. No actual changes except software version and references to other 7.0 documents. |
| | 2016-04-11 | Martin Wallengren Nilsson | Changed Document Template |
| 1.0 | 2017-03-7 | Martin Wallengren Nilsson | Updated for 7.3. No actual changes except software version |
| 1.1 | 2017-09-06 | Alicia Newell | Changed Document Template, removed General Purpose Worklist, and updated implementation version name and class UID. |
| 1.2 | 2017-09-11 | Alicia Newell | Changed document font. Updated footer. |
| 1.3 | 2018-02-21 | Alicia Newell | Updated for 7.5. Added support for Digital X-Ray Image Storage – For Processing and Digital Mammography X-Ray Image Storage – For Processing. |

2. Conformance Statement Overview

The EasyViz Image Display implements the necessary DICOM services to query, retrieve and display CR, CT, DX, MG, MR, PT, RF, SC, US, and XA images. In addition, EasyViz Image Display may be used to: print DICOM instances to a network attached hardcopy device via the General 2D CAM, import DICOM instances from a CD-R/DVD via the EasyViz PACS Workflow Manager, or export DICOM instances to a CD-R/DVD via the EasyViz PACS Workflow Manager.

The DICOM Networking Services supported by the EasyViz Image Display are listed in Table 1.

NETWORK SERVICES

| DICOM SOP Class Name | User of Service (SCU) | Provider of Service (SCP) |
|--|-----------------------|---------------------------|
| Transfer | | |
| Hardcopy Grayscale Image Storage SOP Class (Retired) | Yes | Yes |
| Hardcopy Color Image Storage SOP Class (Retired) | Yes | Yes |
| Computed Radiography Image Storage | Yes | Yes |
| Digital X-Ray Image Storage – For Presentation | Yes | Yes |
| Digital X-Ray Image Storage – For Processing | Yes | Yes |
| Digital Mammography X-Ray Image Storage – For Presentation | Yes | Yes |
| Digital Mammography X-Ray Image Storage – For Processing | Yes | Yes |
| Digital Intra-oral X-Ray Image Storage – For Presentation | Yes | Yes |
| Digital Intra-oral X-Ray Image Storage – For Processing | Yes | No |
| CT Image Storage | Yes | Yes |
| Enhanced CT Image Storage | Yes | Yes |
| Ultrasound Multi-frame Image Storage (Retired) | Yes | Yes |
| Ultrasound Multi-frame Image Storage | Yes | Yes |
| MR Image Storage | Yes | Yes |
| Enhanced MR Image Storage | Yes | Yes |
| Nuclear Medicine Image Storage (Retired) | Yes | Yes |
| Ultrasound Image Storage (Retired) | Yes | Yes |
| Ultrasound Image Storage | Yes | Yes |
| Secondary Capture Image Storage | Yes | Yes |
| Multi-frame Grayscale Byte Secondary Capture Image Storage | Yes | Yes |
| Multi-frame Grayscale Word Secondary Capture Image Storage | Yes | Yes |
| Multi-frame True Color Secondary Capture Image Storage | Yes | Yes |
| Grayscale Softcopy Presentation State Storage SOP Class | Yes | Yes |

| DICOM SOP Class Name | User of Service (SCU) | Provider of Service (SCP) |
|--|-----------------------|---------------------------|
| Color Softcopy Presentation State Storage SOP Class | Yes | Yes |
| Pseudo-Color Softcopy Presentation State Storage SOP Class | Yes | Yes |
| X-Ray Angiographic Image Storage | Yes | Yes |
| Enhanced XA Image Storage | Yes | Yes |
| X-Ray Radiofluoroscopic Image Storage | Yes | Yes |
| Enhanced XRF Image Storage | Yes | Yes |
| Nuclear Medicine Image Storage | Yes | Yes |
| VL Endoscopic Image Storage | Yes | Yes |
| Video Endoscopic Image Storage | Yes | Yes |
| VL Microscopic Image Storage | Yes | Yes |
| Video Microscopic Image Storage | Yes | Yes |
| VL Slide-Coordinates Microscopic Image Storage | Yes | Yes |
| VL Photographic Image Storage | Yes | Yes |
| Video Photographic Image Storage | Yes | Yes |
| Ophthalmic Photographic 8 Bit Image Storage | Yes | Yes |
| Ophthalmic Photographic 16 Bit Image Storage | Yes | Yes |
| Basic Text SR Storage | Yes | Yes |
| Enhanced SR Storage | Yes | Yes |
| Comprehensive SR Storage | Yes | Yes |
| Mammography CAD SR Storage | Yes | Yes |
| Key Object Selection Document | Yes | Yes |
| Positron Emission Tomography Image Storage | Yes | Yes |
| MI 3D Softcopy Presentation State | Yes | Yes |
| | | |
| <i>Query/Retrieve</i> | | |
| Study Root Q/R Information Model – FIND | Yes | No |
| Study Root Q/R Information Model – MOVE | Yes | No |
| | | |
| <i>Print Management</i> | | |
| Basic Grayscale Print Management Meta SOP Class | Yes | No |

| DICOM SOP Class Name | User of Service (SCU) | Provider of Service (SCP) |
|--------------------------------|-----------------------|---------------------------|
| Presentation LUT SOP Class | Yes | No |
| Basic Annotation Box SOP Class | Yes | No |

Table 1: Network Services supported by EasyViz Image Display.

The DICOM Media Services supported by the EasyViz Image Display are listed in Table 2.

| Media Storage Application Profile | Write Files (FSC/FSU) | Read Files (FSR) |
|--|-----------------------|------------------|
| <i>Compact Disk – Recordable</i> | | |
| General Purpose CD-R Interchange | Yes | Yes |
| <i>DVD</i> | | |
| General Purpose Interchange on DVD-RAM Media | Yes | Yes |

Table 2: Media Services supported by EasyViz Image Display.

3. Introduction

3.1 Audience

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

3.2 Remarks

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with EasyViz and other vendors' equipment. The Conformance Statement should be read and understood in conjunction with the DICOM Standard [DICOM]. However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

The comparison of different conformance statements is the first step towards assessing interconnectivity between EasyViz and other vendors' equipment.

Test procedures should be defined to validate the desired level of connectivity.

The DICOM Standard will evolve to meet the users' future requirements. Karos Health reserves the right to make changes to its products or to discontinue its delivery.

3.3 Terms and Abbreviations

Definitions, terms and abbreviations used in this document are defined within the different parts of the DICOM standard. A list of abbreviations and terms can be seen in Table 3.

| Term | Description |
|------|---------------------------------------|
| AE | DICOM Application Entity. |
| AET | Application Entity Title. |
| BSPS | Blending Softcopy Presentation State. |

| Term | Description |
|-------------|---|
| CAD | Computer Aided Diagnostics. |
| CD-R | CD Recordable. |
| CR | Computed Radiography. |
| CT | Computed Tomography. |
| DICOM | Digital Imaging and Communications in Medicine. |
| DX | Digital X-Ray. |
| FSC | File Set Creator. |
| FSU | File Set Updater. |
| FSR | File Set Reader. |
| GSDF | Grayscale Standard Display Function. |
| GSPS | Grayscale Presentation State. |
| MG | Mammography. |
| MR | Magnetic Resonance. |
| PT | Positron Emission Tomography. |
| RF | X-Ray Radiofluoroscopic. |
| SC | Secondary Capture. |
| SCP | DICOM Service Class Provider (DICOM Server). |
| SCU | DICOM Service Class User (DICOM Client). |
| SOP | DICOM Service-Object Pair. |
| US | Ultrasound. |
| XA | X-Ray Angiographic. |

Table 3: Abbreviations and Terms.

3.4 References

| Reference ID | Description |
|---------------------|--|
| | Digital Imaging and Communications in Medicine (DICOM), NEMA PS 3.1-3.20, 2017a. National Electrical Manufacturers Association (NEMA), 1300N 17th Street, Rosslyn, Virginia 22209, USA. |

4. Networking

4.1 Implementation Model

The EasyViz Image Display DICOM Networking Services are implemented in a number of processes launched and terminated by the user.

The EasyViz PACS Workflow Manager, launched at user login, provides DICOM Services to query and transfer DICOM Instances via the Query/Retrieve SCU and the Storage SCU Application Entities.

The EasyViz CAMs, which are launched from the EasyViz PACS Workflow Manager, provides DICOM Services to retrieve and present DICOM Instances via the Query/Retrieve SCU and Storage SCP Application Entities. Moreover, the EasyViz General 2D CAM provides DICOM Services to store Grayscale Softcopy Presentation States, Key Objects and Secondary Captures via the Storage SCU Application Entity and DICOM services related to hardcopy printing via the Print Management SCU Application Entity. The EasyViz General 3D CAM provides DICOM Service to store private SOP-class 3D softcopy presentation states via the Storage SCU Application Entity.

4.1.1 Application Data Flow

Application data flow diagram for the EasyViz Image Display can be seen on Figure 1.

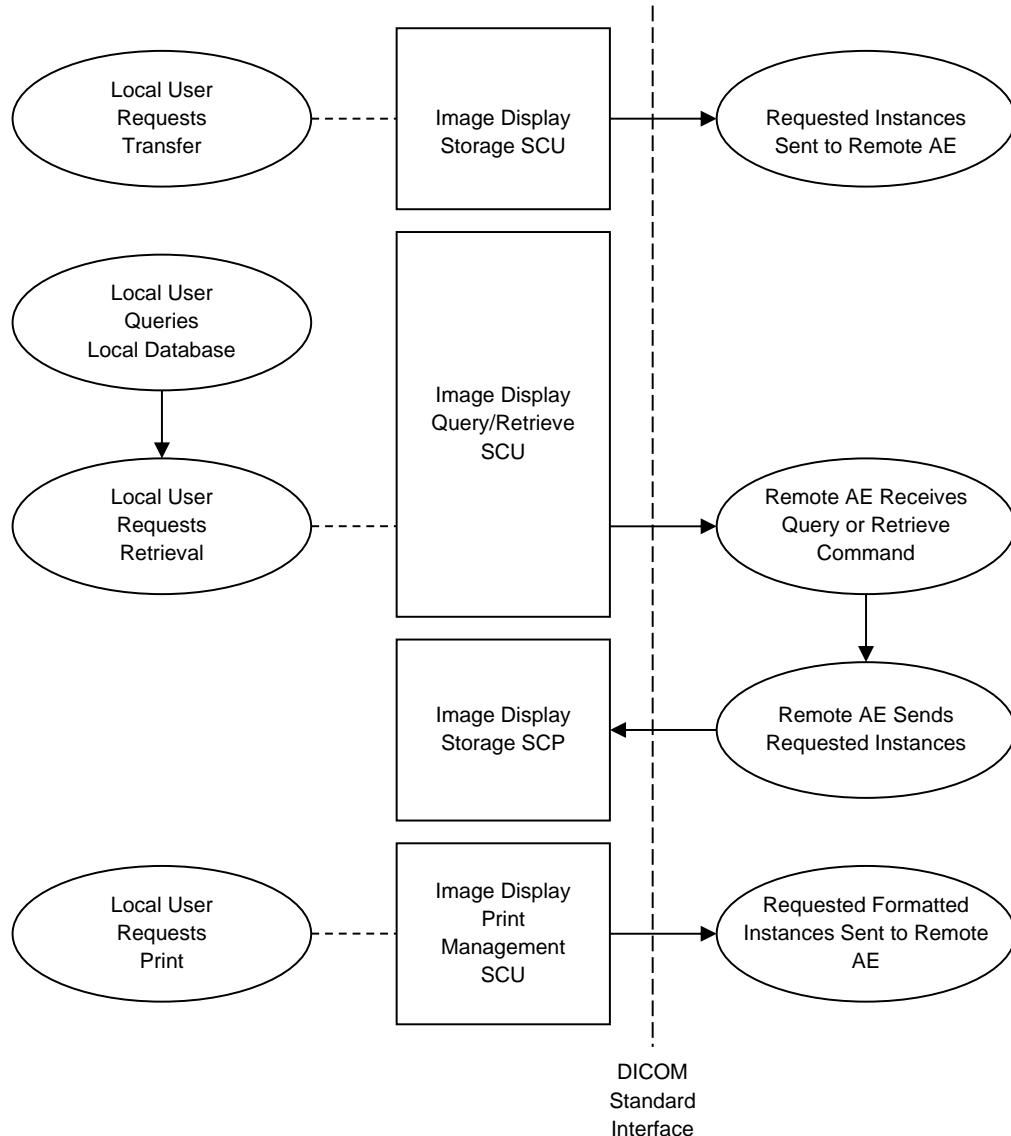


Figure 1: Application Data Flow Diagram.

4.1.2 Functional Definitions of AE's

4.1.2.1 Functional Definition: Query/Retrieve SCU

The Query/Retrieve SCU Application Entity provides DICOM Services to query and retrieve DICOM Instances from remote DICOM Application Entities.

The Query/Retrieve SCU Application Entity does not always query a remote DICOM Application Entities about images before retrieving the images. The Query/Retrieve SCU may also use the information in the internal database to obtain information on available studies. The internal database is updated by EasyViz VPS.

4.1.2.1.1 The Query/Retrieve SCU Application Entity Provides DICOM Services to:

- Query and retrieve DICOM Instances from remote DICOM Application Entities using the DICOM Query/Retrieve SOP (Acting as SCU).

4.1.2.2 Functional Definition: Storage SCU

The Storage SCU Application Entity provides DICOM Services to transfer DICOM Instances to a remote DICOM Application Entity. This Application Entity is intended to be used to transfer DICOM Instances to the local image display, i.e. transfer images from a local CD-ROM/DVD drive to the local archive.

Note: the EasyViz Image Display supports transfer of DICOM Instances, which are not supported for displayed, i.e. the Storage SCU is capable of transferring Nuclear Medicine images, which currently cannot be displayed.

4.1.2.2.1 The Storage SCU Application Entity Provides DICOM Services to:

- Transfer DICOM Instances to a remote DICOM Application Entity using a number of DICOM Image Storage SOPs (Acting as SCU).

4.1.2.3 Functional Definition: Storage SCP

- The Storage SCP Application Entity provides DICOM Services to receive images and other DICOM Instances from remote DICOM Application Entities.

4.1.2.3.1 The Storage SCP Application Entity Provides DICOM Services to:

- Receive DICOM Instances from remote DICOM Application Entities using a number of DICOM Image Storage SOPs (Acting as SCP).

4.1.2.4 Functional Definition: Print Management SCU

The Print Management SCU Application Entity provides DICOM Services to print grayscale images including Presentation LUTs and Annotations on a remote DICOM Application Entity.

4.1.2.4.1 The Print Management SCU Application Entity Provides DICOM Services to:

- Print Grayscale Images incl. an optional Presentation LUT to remote DICOM Application Entities using the DICOM Basic Grayscale Print Management Meta SOP Class (Acting as SCU) and the DICOM Presentation LUT SOP Class (Acting as SCU).
- Print annotations to DICOM peer Application Entities using the DICOM Basic Annotation Box SOP (Acting as SCU).

4.1.3 Sequencing of Real World Activities

The sequencing constraints for the EasyViz Image Display Application Entities can be seen on Figure 2, Figure 3 and Figure 4.

The Query/Retrieve SCU may either query the internal DB or a Peer AE for information on SOP Instances, so either the transaction marked by *) is used or the transaction marked by **), see Figure 2.

The Print Management SCU will not update an instance of the Basic Grayscale Image Box SOP Class before it has been received by the Image Display Storage SCP.

If collation is disabled, the Print Management SCU will send the two transactions marked by *), otherwise the two transactions marked by **) are sent – see Figure 3.

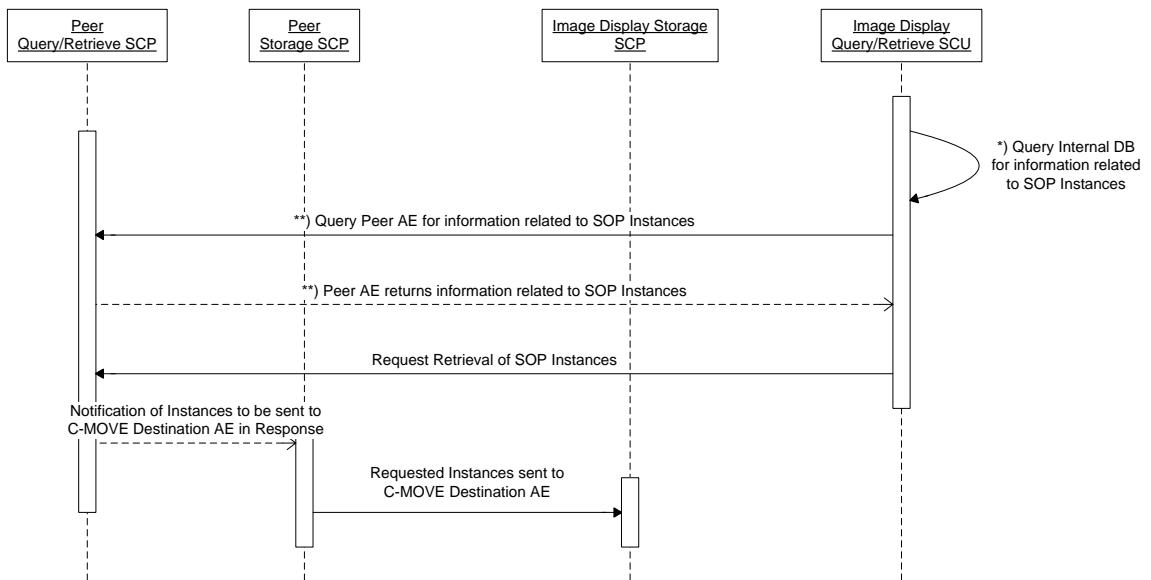


Figure 2: Storage SCP and Query/Retrieve SCU: Sequencing Constraints.

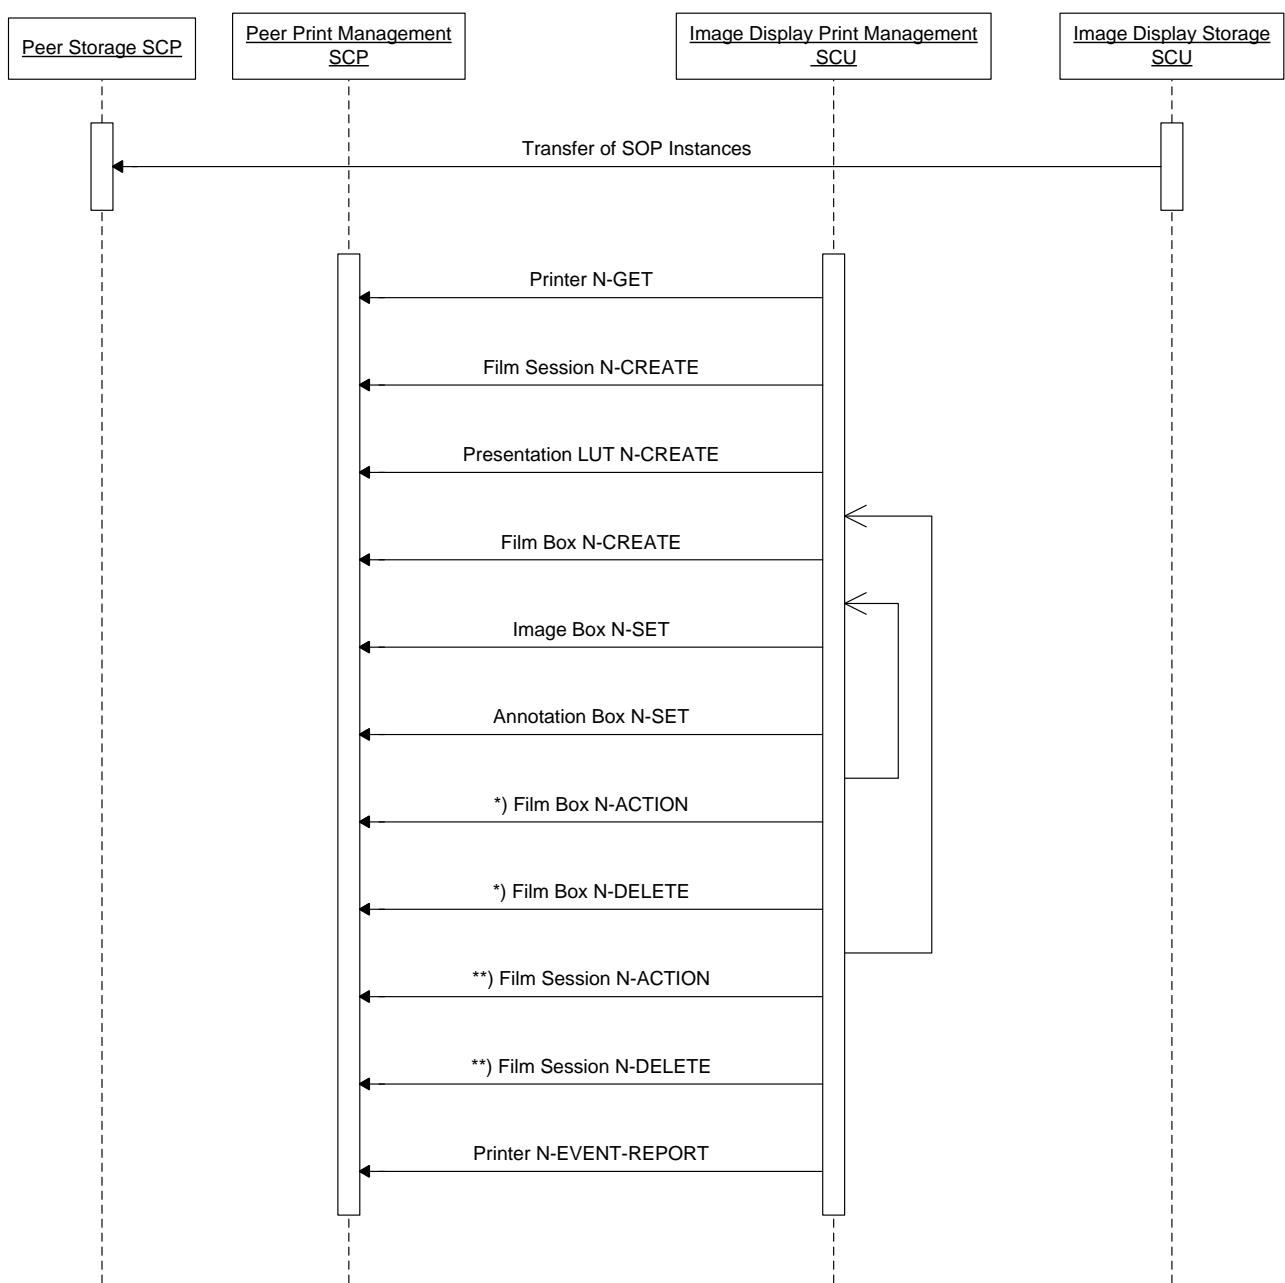


Figure 3: Storage SCU and Print Management SCU: Sequencing Constraints.

4.1.4 AE Specification: Query/Retrieve SCU

4.1.4.1 SOP Classes

The Query/Retrieve SCU provides Standard Conformance to the SOP Classes listed in Table 4.

| SOP Class Name | SOP Class UID | SCU | SCP |
|---|-----------------------------|-----|-----|
| <i>Query/Retrieve</i> | | | |
| Study Root Q/R Information Model - FIND | 1.2.840.10008.5.1.4.1.2.2.1 | Yes | No |
| Study Root Q/R Information Model – MOVE | 1.2.840.10008.5.1.4.1.2.2.2 | Yes | No |

Table 4: Query/Retrieve SCU: Supported SOP Classes.

4.1.4.2 Association Policies

4.1.4.2.1 General

The Query/Retrieve SCU will propose Association Requests for DICOM Query/Retrieve Service. The DICOM standard application context name for DICOM 3.0 is always proposed, see Table 5.

| | |
|--------------------------|-----------------------|
| Application Context Name | 1.2.840.10008.3.1.1.1 |
|--------------------------|-----------------------|

Table 5: Query/Retrieve SCU: DICOM Application Context.

4.1.4.2.2 Number of Associations

The Query/Retrieve SCU does not support multiple simultaneous associations, see Table 6.

| | |
|---|-------------------|
| Maximum number of simultaneous associations | 1 – Configurable. |
|---|-------------------|

Table 6: Query/Retrieve SCU: Number of simultaneous associations.

4.1.4.2.3 Asynchronous Nature

The Query/Retrieve SCU does not support asynchronous communication. Multiple outstanding transactions are not supported, see Table 7.

| | |
|---|-------------------|
| Maximum number of outstanding asynchronous transactions | 1 – Configurable. |
|---|-------------------|

Table 7: Query/Retrieve SCU: Asynchronous nature.

4.1.4.2.4 Implementation Identifying Information

The identifying information for the Query/Retrieve SCU can be seen in Table 8.

| | |
|-----------------------------|------------------------------|
| Implementation Class UID | 1.3.6.1.4.1.16978.0.3.5.4.31 |
| Implementation Version Name | EV-3.5.4-31 |

Table 8: Query/Retrieve SCU: DICOM Implementation Class and Version.

4.1.4.3 Association Initiation Policy

4.1.4.3.1 Activity: Query Instances

4.1.4.3.1.1 Description and Sequencing of Activities

The Query/Retrieve SCU sends an Association Request to a remote DICOM Application Entity acting as Query/Retrieve SCP when the user queries a PACS from the EasyViz Workflow Manager. Note that by default, worklist in the EasyViz Workflow Manager are populated using the internal database. Sequencing constraints for the Query Instances activity can be seen in Figure 2.

4.1.4.3.1.2 Proposed Presentation Contexts

The Query/Retrieve SCU will propose the Presentation Context listen in Table 9: Query/Retrieve SCU: Proposed Presentation Contexts for the Query Instances activity for the Query Instances activity.

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|---|-----------------------------|--|---|------|----------------------|
| Name | UID | Name List | UID List | | |
| Study Root Q/R Information Model – FIND | 1.2.840.10008.5.1.4.1.2.2.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | Relational-retrieval |

Table 9: Query/Retrieve SCU: Proposed Presentation Contexts for the Query Instances activity.

4.1.4.3.1.3 Extended Negotiation

The Query/Retrieve SCU will try to negotiate Relational-Retrieval with the Peer Application Entity acting as Query/Retrieve SCP. If the Query/Retrieve SCU fails to negotiate Relational-Retrieval, then only baseline SCU behavior is performed.

4.1.4.3.2 Activity: Retrieve Instances

4.1.4.3.2.1 Description and Sequencing of Activities

The Query/Retrieve SCU sends an Association Request to a remote DICOM Application Entity acting as Query/Retrieve SCP when the user launches a CAM from the EasyViz Workflow Manager. Sequencing constraints for the Retrieve Instances activity can be seen in Figure 2.

4.1.4.3.2.2 Proposed Presentation Contexts

The Query/Retrieve SCU will propose the Presentation Contexts listed in Table 10 for the Retrieve Instances activity.

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|---|-----------------------------|--|---|------|----------------------|
| Name | UID | Name List | UID List | | |
| Study Root Q/R Information Model – MOVE | 1.2.840.10008.5.1.4.1.2.2.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | Relational-retrieval |

Table 10: Query/Retrieve SCU: Proposed Presentation Contexts for the Retrieve Instances activity.

4.1.4.3.2.3 Extended Negotiation

The Query/Retrieve SCU will try to negotiate Relational-Retrieval with the Peer Application Entity acting as Query/Retrieve SCP. If the Query/Retrieve SCU fails to negotiate Relational-Retrieval with the Query/Retrieve SCP, then only baseline SCU behavior is performed.

4.1.4 Association Acceptance Policy

The Query/Retrieve SCU does not accept associations.

4.1.5 AE Specification: Storage SCU

4.1.5.1 SOP Classes

The Storage SCU provides Standard Conformance to the SOP Classes listed in Table 11.

| SOP Class Name | SOP Class UID | SCU | SCP |
|--|---------------------------|-----|-----|
| <i>Transfer</i> | | | |
| Hardcopy Grayscale Image Storage SOP Class | 1.2.840.10008.5.1.1.29 | Yes | No |
| Hardcopy Color Image Storage SOP Class | 1.2.840.10008.5.1.1.30 | Yes | No |
| Computed Radiography Image Storage | 1.2.840.10008.5.1.4.1.1.1 | Yes | No |

| SOP Class Name | SOP Class UID | SCU | SCP |
|--|--------------------------------|-----|-----|
| Digital X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.1 | Yes | No |
| Digital X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.1 | Yes | No |
| Digital Mammography X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.2 | Yes | No |
| Digital Mammography X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.2.1 | Yes | No |
| Breast Tomosynthesis Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.13.1.3 | Yes | No |
| Digital Intra-oral X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.3 | Yes | No |
| Digital Intra-oral X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.3.1 | Yes | No |
| CT Image Storage | 1.2.840.10008.5.1.4.1.1.2 | Yes | No |
| Enhanced CT Image Storage | 1.2.840.10008.5.1.4.1.1.2.1 | Yes | No |
| Ultrasound Multi-frame Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.3 | Yes | No |
| Ultrasound Multi-frame Image Storage | 1.2.840.10008.5.1.4.1.1.3.1 | Yes | No |
| MR Image Storage | 1.2.840.10008.5.1.4.1.1.4 | Yes | No |
| Enhanced MR Image Storage | 1.2.840.10008.5.1.4.1.1.4.1 | Yes | No |
| Nuclear Medicine Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.5 | Yes | No |
| Ultrasound Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.6 | Yes | No |
| Ultrasound Image Storage | 1.2.840.10008.5.1.4.1.1.6.1 | Yes | No |
| Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7 | Yes | No |
| Multi-frame Grayscale Byte Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7.2 | Yes | No |
| Multi-frame Grayscale Word Secondary Capture Image Store | 1.2.840.10008.5.1.4.1.1.7.3 | Yes | No |
| Multi-frame True Color Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7.4 | Yes | No |
| Grayscale Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.1 | Yes | No |
| Color Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.2 | Yes | No |
| Pseudo-Color Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.3 | Yes | No |
| X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1 | Yes | No |

| SOP Class Name | SOP Class UID | SCU | SCP |
|--|----------------------------------|-----|-----|
| Enhanced X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1.1 | Yes | No |
| X-Ray Radiofluoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2 | Yes | No |
| Enhanced X-Ray Radiofluoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2.1 | Yes | No |
| Nuclear Medicine Image Storage | 1.2.840.10008.5.1.4.1.1.20 | Yes | No |
| VL Endoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.1 | Yes | No |
| Video Endoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.1.1 | Yes | No |
| VL Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.2 | Yes | No |
| Video Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.2.1 | Yes | No |
| VL Slide-Coordinates Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.3 | Yes | No |
| VL Photographic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.4 | Yes | No |
| Video Photographic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.4.1 | Yes | No |
| Ophthalmic Photographic 8 Bit Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.5.1 | Yes | No |
| Ophthalmic Photographic 16 Bit Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.5.2 | Yes | No |
| Basic Text SR Storage | 1.2.840.10008.5.1.4.1.1.88.11 | Yes | No |
| Enhanced SR Storage | 1.2.840.10008.5.1.4.1.1.88.22 | Yes | No |
| Comprehensive SR Storage | 1.2.840.10008.5.1.4.1.1.88.33 | Yes | No |
| Mammography CAD SR Storage | 1.2.840.10008.5.1.4.1.1.88.50 | Yes | No |
| Key Object Selection Document | 1.2.840.10008.5.1.4.1.1.88.59 | Yes | No |
| Positron Emission Tomography Image Storage | 1.2.840.10008.5.1.4.1.1.128 | Yes | No |
| MI 3D Softcopy Presentation State | 1.3.6.1.4.1.16978.3.1 | Yes | No |

Table 11: Storage SCU: Supported SOP Classes.

4.1.5.2 Association Policies

4.1.5.2.1 General

The Storage SCU will propose Association Requests for DICOM Storage Services. The DICOM standard application context name for DICOM 3.0 is always proposed, see Table 12.

| | |
|--------------------------|-----------------------|
| Application Context Name | 1.2.840.10008.3.1.1.1 |
|--------------------------|-----------------------|

Table 12: Storage SCU: DICOM Application Context.

4.1.5.2.2 Number of Associations

The Storage SCU does not support multiple simultaneous associations, see Table 13.

| | |
|---|-------------------|
| Maximum number of simultaneous associations | 1 – Configurable. |
|---|-------------------|

Table 13: Storage SCU: Number of simultaneous associations.

4.1.5.2.3 Asynchronous Nature

The Storage SCU does not support asynchronous communication. Multiple outstanding transactions are not supported, see Table 14.

| | |
|---|-------------------|
| Maximum number of outstanding asynchronous transactions | 1 – Configurable. |
|---|-------------------|

Table 14: Storage SCU: Asynchronous nature.

4.1.5.2.4 Implementation Identifying Information

The identifying information for the Storage SCU can be seen in Table 15.

| | |
|-----------------------------|------------------------------|
| Implementation Class UID | 1.3.6.1.4.1.16978.0.3.5.4.31 |
| Implementation Version Name | EV-3.5.4-31 |

Table 15: Storage SCU: DICOM Implementation Class and Version.

4.1.5.3 Association Initiation Policy

4.1.5.3.1 Activity: Transfer Instances

4.1.5.3.1.1 Description and Sequencing of Activities

The Storage SCU sends an Association Request to a remote DICOM Application Entity acting as Storage SCP when the selects import in the EasyViz Workflow Manager. This is intended to be used to import selected DICOM Instances from CD-ROM/DVD to the local archive.

4.1.5.3.1.2 Proposed Presentation Contexts

The Storage SCU will propose the Presentation Contexts listed in Table 16 for the Transfer Instances activity.

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|--------------------------------|---|---|------|----------|
| Name | UID | Name List | UID List | | |
| Hardcopy Grayscale Image Storage SOP Class | 1.2.840.10008.5.1.1.29 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Hardcopy Color Image Storage SOP Class | 1.2.840.10008.5.1.1.30 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Computed Radiography Image Storage | 1.2.840.10008.5.1.4.1.1.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Digital X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Digital X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.1.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Digital Mammography X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.2 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Digital Mammography X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.2.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Breast Tomosynthesis Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.13.1.3 | Implicit VR LittleEndian Explicit VR LittleEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 | SCU | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|-----------------------------|--|---|------|----------|
| Name | UID | Name List | UID List | | |
| | | Explicit VR Big Endian | 1.2.840.10008.1.2.2 | | |
| Digital Intra-oral X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Digital Intra-oral X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.3.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| CT Image Storage | 1.2.840.10008.5.1.4.1.1.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Enhanced CT Image Storage | 1.2.840.10008.5.1.4.1.1.2.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Ultrasound Multi-frame Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Ultrasound Multi-frame Image Storage | 1.2.840.10008.5.1.4.1.1.3.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| MR Image Storage | 1.2.840.10008.5.1.4.1.1.4 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Enhanced MR Image Storage | 1.2.840.10008.5.1.4.1.1.4.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Nuclear Medicine Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.5 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Ultrasound Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.6 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Ultrasound Image Storage | 1.2.840.10008.5.1.4.1.1.6.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Multi-frame Grayscale Byte Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Multi-frame Grayscale Word Secondary Capture Image Store | 1.2.840.10008.5.1.4.1.1.7.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Multi-frame True Color Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7.4 | Implicit VR Little Endian Explicit VR Little Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 | SCU | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|----------------------------------|--|---|------|----------|
| Name | UID | Name List | UID List | | |
| | | Explicit VR Big Endian | 1.2.840.10008.1.2.2 | | |
| Grayscale Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Color Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Pseudo-Color Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Enhanced X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| X-Ray Radiofluoroscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Enhanced X-Ray Radiofluoroscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Nuclear Medicine Image Storage | 1.2.840.10008.5.1.4.1.1.20 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| VL Endoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Video Endoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| VL Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Video Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.2.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| VL Slide-Coordinates Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| VL Photographic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.4 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Video Photographic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.4.1 | Implicit VR Little Endian Explicit VR Little Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 | SCU | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|----------------------------------|--|---|------|----------|
| Name | UID | Name List | UID List | | |
| | | Explicit VR Big Endian | 1.2.840.10008.1.2.2 | | |
| Ophthalmic Photographic 8 Bit Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.5.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Ophthalmic Photographic 16 Bit Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.5.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Basic Text SR | 1.2.840.10008.5.1.4.1.1.88.11 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Enhanced SR | 1.2.840.10008.5.1.4.1.1.88.22 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Comprehensive SR | 1.2.840.10008.5.1.4.1.1.88.33 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Mammography CAD SR | 1.2.840.10008.5.1.4.1.1.88.50 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Key Object Selection Document | 1.2.840.10008.5.1.4.1.1.88.59 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Positron Emission Tomography Image Storage | 1.2.840.10008.5.1.4.1.1.128 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| MI 3D Softcopy Presentation State | 1.3.6.1.4.1.1.16978.3.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |

Table 16: Storage SCU: Proposed Presentation Contexts for the Transfer Instances activity.

4.1.5.3.1.3 Extended Negotiation

No extended negotiation is performed.

4.1.5.4 Association Acceptance Policy

The Storage SCU does not accept associations.

4.1.6 AE Specification: Storage SCP

4.1.6.1 SOP Classes

The Storage SCP provides Standard Conformance to the SOP Classes listed in Table 17.

| SOP Class Name | SOP Class UID | SCU | SCP |
|--|------------------------|-----|-----|
| Transfer | | | |
| Hardcopy Grayscale Image Storage SOP Class (Retired) | 1.2.840.10008.5.1.1.29 | No | Yes |

| SOP Class Name | SOP Class UID | SCU | SCP |
|--|--------------------------------|-----|-----|
| Hardcopy Color Image Storage SOP Class (Retired) | 1.2.840.10008.5.1.1.30 | No | Yes |
| Computed Radiography Image Storage | 1.2.840.10008.5.1.4.1.1.1 | No | Yes |
| Digital X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.1 | No | Yes |
| Digital X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.1.1 | No | Yes |
| Digital Mammography X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.2 | No | Yes |
| Digital Mammography X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.2.1 | No | Yes |
| Breast Tomosynthesis Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.13.1.3 | No | Yes |
| Digital Intra-oral X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.3 | No | Yes |
| CT Image Storage | 1.2.840.10008.5.1.4.1.1.2 | No | Yes |
| Enhanced CT Image Storage | 1.2.840.10008.5.1.4.1.1.2.1 | No | Yes |
| Ultrasound Multi-frame Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.3 | No | Yes |
| Ultrasound Multi-frame Image Storage | 1.2.840.10008.5.1.4.1.1.3.1 | No | Yes |
| MR Image Storage | 1.2.840.10008.5.1.4.1.1.4 | No | Yes |
| Enhanced MR Image Storage | 1.2.840.10008.5.1.4.1.1.4.1 | No | Yes |
| Nuclear Medicine Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.5 | No | Yes |
| Ultrasound Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.6 | No | Yes |
| Ultrasound Image Storage | 1.2.840.10008.5.1.4.1.1.6.1 | No | Yes |
| Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7 | No | Yes |
| Multi-frame Grayscale Byte Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7.2 | No | Yes |
| Multi-frame Grayscale Word Secondary Capture Image Store | 1.2.840.10008.5.1.4.1.1.7.3 | No | Yes |
| Multi-frame True Color Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7.4 | No | Yes |
| Grayscale Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.1 | No | Yes |
| Color Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.2 | No | Yes |

| SOP Class Name | SOP Class UID | SCU | SCP |
|--|----------------------------------|-----|-----|
| Pseudo-Color Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.3 | No | Yes |
| X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1 | No | Yes |
| Enhanced X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1.1 | No | Yes |
| X-Ray Radiofluoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2 | No | Yes |
| Enhanced X-Ray Radiofluoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2.1 | No | Yes |
| Nuclear Medicine Image Storage | 1.2.840.10008.5.1.4.1.1.20 | No | Yes |
| VL Image Storage (retired) | 1.2.840.10008.5.1.4.1.1.77.1 | No | Yes |
| VL Endoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.1 | No | Yes |
| Video Endoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.1.1 | No | Yes |
| VL Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.2 | No | Yes |
| Video Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.2.1 | No | Yes |
| VL Slide-Coordinates Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.3 | No | Yes |
| VL Photographic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.4 | No | Yes |
| Video Photographic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.4.1 | No | Yes |
| Ophthalmic Photographic 8 Bit Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.5.1 | No | Yes |
| Ophthalmic Photographic 16 Bit Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.5.2 | No | Yes |
| Basic Text SR Storage | 1.2.840.10008.5.1.4.1.1.88.11 | No | Yes |
| Enhanced SR Storage | 1.2.840.10008.5.1.4.1.1.88.22 | No | Yes |
| Comprehensive SR Storage | 1.2.840.10008.5.1.4.1.1.88.33 | No | Yes |
| Mammography CAD SR Storage | 1.2.840.10008.5.1.4.1.1.88.50 | No | Yes |
| Key Object Selection Document | 1.2.840.10008.5.1.4.1.1.88.59 | No | Yes |
| Positron Emission Tomography Image Storage | 1.2.840.10008.5.1.4.1.1.128 | No | Yes |
| MI 3D Softcopy Presentation State | 1.3.6.1.4.1.16978.3.1 | No | Yes |

Table 17: Storage SCP: Supported SOP Classes.

4.1.6.2 Association Policies

4.1.6.2.1 General

The Storage SCP will accept Association Requests for DICOM Storage Services. The DICOM standard application context name for DICOM 3.0 is always accepted, see Table 18.

| | |
|--------------------------|-----------------------|
| Application Context Name | 1.2.840.10008.3.1.1.1 |
|--------------------------|-----------------------|

Table 18: Storage SCP: DICOM Application Context.

4.1.6.2.2 Number of Associations

The Storage SCP does not support multiple simultaneous associations, see Table 19.

| | |
|---|-------------------|
| Maximum number of simultaneous associations | 1 – Configurable. |
|---|-------------------|

Table 19: Storage SCP: Number of simultaneous associations.

4.1.6.2.3 Asynchronous Nature

The Storage SCP does not support asynchronous communication. Multiple outstanding transactions are not supported, see Table 20.

| | |
|---|-------------------|
| Maximum number of outstanding asynchronous transactions | 1 – Configurable. |
|---|-------------------|

Table 20: Storage SCP: Asynchronous nature.

4.1.6.2.4 Implementation Identifying Information

The identifying information for the Storage SCP can be seen in Table 21.

| | |
|-----------------------------|------------------------------|
| Implementation Class UID | 1.3.6.1.4.1.16978.0.3.5.4.31 |
| Implementation Version Name | EV-3.5.4-31 |

Table 21: Storage SCP: DICOM Implementation Class and Version.

4.1.6.3 Association Initiation Policy

The Storage SCP does not initiate associations.

4.1.6.4 Association Acceptance Policy

4.1.6.4.1 Activity: Receive Instances

4.1.6.4.1.1 Description and Sequencing of Activities

A remote DICOM Application Entity acting as a Storage SCU may establish an association with the Storage SCP. The Storage SCP will accept these associations for the purpose of receiving supported SOP Class Instances.

When the user launches a CAM from the EasyViz Workflow Manager, the CAM will initiate the Retrieve Instances activity as described in section 3.1.4.3. The C-MOVE request in the Retrieve Instances activity contains the Storage SCP as destination Application Entity.

4.1.6.4.1.2 Accepted Presentation Contexts

The Storage SCP accepts the Application Presentation Contexts listed in Table 22.

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|------------------------|--|---|------|----------|
| Name | UID | Name List | UID List | | |
| Hardcopy Grayscale Image Storage SOP Class (Retired) | 1.2.840.10008.5.1.1.29 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|---------------------------|---|---|------|----------|
| Name | UID | Name List | UID List | | |
| | | | 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| Hardcopy Color Image Storage SOP Class (Retired) | 1.2.840.10008.5.1.1.30 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 | SCP | None |
| Computed Radiography Image Storage | 1.2.840.10008.5.1.4.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 | SCP | None |
| Digital X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|-----------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| | | Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| Digital X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Digital Mammography X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Digital Mammography X-Ray Image | 1.2.840.10008.5.1.4.1.1.2.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|---|--------------------------------|--|--|------|-------------|
| Name | UID | Name List | UID List | | |
| Storage – For Processing | | JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| Breast Tomosynthesis Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.13.1.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Digital Intra-oral X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|-----------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| | | | 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| CT Image Storage | 1.2.840.10008.5.1.4.1.1.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Enhanced CT Image Storage | 1.2.840.10008.5.1.4.1.1.2.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Ultrasound Multi-frame Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--------------------------------------|-----------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| | | Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| Ultrasound Multi-frame Image Storage | 1.2.840.10008.5.1.4.1.1.3.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| MR Image Storage | 1.2.840.10008.5.1.4.1.1.4 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Enhanced MR Image Storage | 1.2.840.10008.5.1.4.1.1.4.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|---------------------------|---|--|------|-------------|
| Name | UID | Name List | UID List | | |
| | | JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| Nuclear Medicine Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.5 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Ultrasound Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.6 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|-----------------------------|--|---|------|-------------|
| Name | UID | Name List | UID List | | |
| Ultrasound Image Storage | 1.2.840.10008.5.1.4.1.1.6.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2.4.91 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Multi-frame Grayscale Byte Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 | | |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|------------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| | | JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| Multi-frame Grayscale Word Secondary Capture Image Store | 1.2.840.10008.5.1.4.1.1.7.3 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| Multi-frame True Color Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7.4 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| Grayscale Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCP | None |
| Color Softcopy Presentation State | 1.2.840.10008.5.1.4.1.1.11.2 | Implicit VR LittleEndian Explicit VR LittleEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|--------------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| Storage SOP Class | | Explicit VR Big Endian | 1.2.840.10008.1.2.2 | | |
| Pseudo-Color Softcopy Presentation State Storage SOP Class | 1.2.840.10008.5.1.4.1.1.11.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCP | None |
| X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Enhanced X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| X-Ray Radiofluoroscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|------------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| | | JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| Enhanced X-Ray Radiofluoroscopic Image Storage | 1.2.840.10008.5.1.4.1.12.2.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Nuclear Medicine Image Storage | 1.2.840.10008.5.1.4.1.1.20 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--------------------------------|----------------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| VL Image Storage (retired) | 1.2.840.10008.5.1.4.1.1.77.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| VL Endoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Video Endoscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|----------------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| | | JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| VL Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Video Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.2.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| VL Slide-Coordinates Microscopic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|----------------------------------|----------------------------------|---|--|------|----------|
| Name | UID | Name List | UID List | | |
| | | JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | | |
| VL Photographic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.4 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Video Photographic Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.4.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|----------------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| Ophthalmic Photographic 8 Bit Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.5.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Ophthalmic Photographic 16 Bit Image Storage | 1.2.840.10008.5.1.4.1.1.77.1.5.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| Basic Text SR | 1.2.840.10008.5.1.4.1.1.88.11 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCP | None |
| Enhanced SR | 1.2.840.10008.5.1.4.1.1.88.22 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCP | None |
| Comprehensive SR | 1.2.840.10008.5.1.4.1.1.88.33 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCP | None |
| Mammography CAD SR | 1.2.840.10008.5.1.4.1.1.88.50 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCP | None |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|-------------------------------|--|--|------|----------|
| Name | UID | Name List | UID List | | |
| Key Object Selection Document | 1.2.840.10008.5.1.4.1.1.88.59 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCP | None |
| Positron Emission Tomography Image Storage | 1.2.840.10008.5.1.4.1.1.128 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian JPEG Baseline (Process 1) JPEG Extended (Process 2 & 4) JPEG Lossless, Non-Hierarchical (Process 14) JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 SV1) JPEG-LS Lossless Image Compression JPEG-LS Lossy (Near-Lossless) Image Compression RLE Lossless JPEG 2000 Lossless only JPEG 2000 Lossless or Lossy | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.57 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.4.80 1.2.840.10008.1.2.4.81 1.2.840.10008.1.2.5 1.2.840.10008.1.2.4.90 1.2.840.10008.1.2.4.91 | SCP | None |
| MI 3D Softcopy Presentation State | 1.3.6.1.4.1.16978.3.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCP | None |

Table 22: Storage SCP: Accepted Presentation Contexts for the Receive Instances activity.

4.1.6.4.1.3 Extended Negotiation

No extended negotiation is performed.

4.1.7 AE Specification: Print Management SCU

4.1.7.1 SOP Classes

The Print Management SCU provides Standard Conformance to SOP Classes listed in Table 23.

| SOP Class Name | SOP Class UID | SCU | SCP |
|---|------------------------|-----|-----|
| <i>Print Management</i> | | | |
| Basic Grayscale Print Management Meta SOP Class | 1.2.840.10008.5.1.1.9 | Yes | No |
| Basic Annotation Box SOP Class | 1.2.840.10008.5.1.1.15 | Yes | No |
| Presentation LUT SOP Class | 1.2.840.10008.5.1.1.23 | Yes | No |

Table 23: Print Management SCU: Supported SOP Classes.

4.1.7.2 Association Policies

4.1.7.2.1 General

The Print Management SCU will propose Association Requests for DICOM Print Management Services. The DICOM standard application context name for DICOM 3.0 is always proposed, see Table 24.

| | |
|--------------------------|-----------------------|
| Application Context Name | 1.2.840.10008.3.1.1.1 |
|--------------------------|-----------------------|

Table 24: Print Management SCU: DICOM Application Context.

4.1.7.2.2 Number of Associations

The Print Management SCU does not support multiple simultaneous associations, see Table 25.

| | |
|---|-------------------|
| Maximum number of simultaneous associations | 1 – Configurable. |
|---|-------------------|

Table 25: Print Management SCU: Number of simultaneous associations.

4.1.7.2.3 Asynchronous Nature

The Print Management SCU does not support asynchronous communication. Multiple outstanding transactions are not supported.

| | |
|---|-------------------|
| Maximum number of outstanding asynchronous transactions | 1 – Configurable. |
|---|-------------------|

Table 26: Print Management SCU: Asynchronous nature.

4.1.7.2.4 Implementation Identifying Information

The identifying information for the Print Management SCU can be seen in Table 27.

| | |
|-----------------------------|------------------------------|
| Implementation Class UID | 1.3.6.1.4.1.16978.0.3.5.4.31 |
| Implementation Version Name | EV-3.5.4-31 |

Table 27: Print Management SCU: DICOM Implementation Class and Version.

4.1.7.3 Association Initiation Policy

4.1.7.3.1 Activity: Print Images

4.1.7.3.1.1 Description and Sequencing of Activities

The Print Management SCU sends an Association Request to a remote DICOM Application Entity acting as Basic Grayscale Print Management Meta SOP Class SCP when the user prints DICOM Instances from the EasyViz General 2D CAM.

4.1.7.3.1.2 Proposed Presentation Contexts

The Print Management SCU will propose Presentation Contexts as listed in Table 28 for the Print Images activity.

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|---|------------------------|---|---|------|----------|
| Name | UID | Name List | UID List | | |
| Basic Grayscale Print Management Meta SOP Class | 1.2.840.10008.5.1.1.9 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Basic Annotation Box SOP Class | 1.2.840.10008.5.1.1.15 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |
| Presentation LUT SOP Class | 1.2.840.10008.5.1.1.23 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | SCU | None |

Table 28: Print Management SCU: Proposed Presentation Contexts for the Print Images activity.

4.1.7.4 Association Acceptance Policy

The Print Management SCU does not accept Association Requests.

4.2 Network Interfaces

4.2.1 Physical Network Interface

The EasyViz Image Display Application Entities are indifferent to the physical medium over which TCP/IP is executed. This is entirely dependent on the underlying operating system and hardware.

4.2.2 Additional Protocols

When hostnames rather than IP addresses are used to specify presentation addresses for remote Application Entities, the EasyViz Image Display Application Entities depends on the name resolution mechanism of the underlying operating system for proper operation.

4.3 Configuration

4.3.1 AE Title/Presentation Address Mapping

4.3.1.1 Local AE Titles

The default Application Entity title and port number of the EasyViz Image Display Application Entities are listed in Table 29.

The default AE Title for the Storage SCP is created from the hostname and port number of the host where the Storage SCP is installed.

| Application Entity | Default AE Title | Default Port Number |
|----------------------|----------------------|---------------------|
| Query/Retrieve SCU | ID_QR_SCU | N/A |
| Storage SCU | ID_STORE_SCU | N/A |
| Storage SCP | <hostname>-<port nr> | 7000 |
| Print Management SCU | ID_PM_SCU | N/A |

Table 29: Local AE Titles.

4.3.1.2 Remote AE Title/Presentation Address Mapping

4.3.1.2.1 Remote Query/Retrieve SCP and Storage SCP

The remote Query/Retrieve SCP and Storage SCP configuration is stored in the environment variable EV_PACS. The EasyViz Image Display assumes that the Query/Retrieve SCP and Storage SCP are located on the same host.

The EV_PACS environment variable has the following structure:

```
hostname=<hostname>,port=<port number>,qr_aet=<aet>,store_aet=<aet>
```

4.3.1.2.2 Remote Print Management SCP

The Print Management SCP configuration is stored in a printer profile in the internal database. For more information on how to setup a printer, see Color Softcopy Presentation State Storage SOP Class

4.3.2 Parameters

The configurable parameters of EasyViz Image Display are listed in Table 30.

| Parameter | Configurable | Default Value |
|--|--------------|---------------|
| <i>General Parameters</i> | | |
| PDU Size | No | 32Kb |
| Time-out waiting for acceptance or rejection Response of an Association Open Request (Application level timeout) | No | None |
| General DIMSE level time-out values | No | None |

| Parameter | Configurable | Default Value |
|--|--------------|--|
| Time-out waiting for response to TCP/IP connect request (Low-level timeout) | Yes | 180s [OS Specific] |
| Time-out waiting for acceptance of a TCP/IP message over the network (Low-level timeout) | Yes | 180s [OS Specific] |
| Time-out waiting for data between TCP/IP packets (Low-level timeout) | Yes | Adaptive 0.2-120s [OS Specific] |
| Any changes to default TCP/IP setting such as configurable stack parameters | No | None |
| <i>AE Specific Parameters</i> | | |
| Size constraint in maximum object size | No | None |
| Maximum PDU Size that the AE can receive | No | 32Kb |
| Maximum PDU Size that the AE can send | No | 32Kb |
| AE specific DIMSE level time-out values | No | None |
| SOP Class Support | No | All supported SOP Classes always proposed and accepted |
| Transfer Syntax Support | No | All supported Transfer Syntaxes always proposed and accepted |

Table 30: Configurable Parameters.

5. Media Interchange

5.1 Implementation Model

The EasyViz Image Display DICOM Media Interchange Services are implemented in two logical Application Entities: the Media FSR Application Entity, and the Media FSC Application Entity.

The Media FSR Application Entity is a logical Application Entity implemented in the EasyViz Workflow Manager. The Media FSR Application Entity, launched at user login, provides DICOM Media Interchange Services to read DICOM Instances from a DICOM Storage Medium such as CD-ROM or DVD.

The Media FSC Application Entity is a logical Application Entity implemented in the EasyViz Workflow Manager. The Media FSC Application Entity provides DICOM Media Interchange Service to write DICOM Instances to a DICOM Storage Medium.

5.1.1 Application Data Flow Diagram

Application data flow diagram for the DICOM Media Interchange Services of the EasyViz Image Display can be seen in Figure 6.

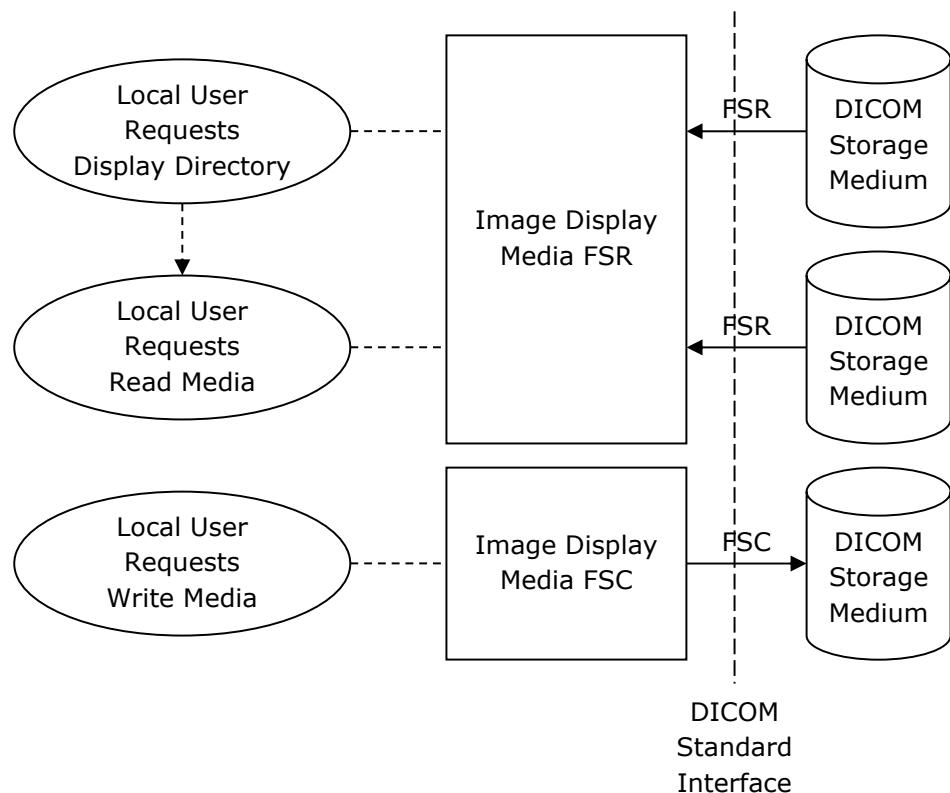


Figure 6: Application Data Flow Diagram.

5.1.2 Functional Definitions of AE's

5.1.2.1 Functional Definition: Media FSR

The Media FSR Application Entity provides DICOM Services to read DICOM files from a DICOM Storage Medium.

5.1.2.1.1 The Media FSR Application Entity Provides DICOM Services to:

- Read DICOM Instances from a DICOM Storage Medium using the DICOM Interchange option of the Media Storage SOP Class (Acting as FSR).

5.1.2.2 Functional Definition: Media FSC

- The Media FSC Application Entity provides DICOM Services to write DICOM files to a DICOM Storage Medium.

5.1.2.2.1 The Media FSC Application Entity Provides DICOM Services to:

- Write DICOM Instances to a DICOM Storage Medium using the DICOM Interchange option of the Media Storage SOP Class (Acting as FSC).

5.1.3 Sequencing of Real World Activities

The sequencing of the DICOM Media Interchange activities for the EasyViz Image Display Application Entities can be seen in Figure 7.

The DICOM Network Application Entity, Storage SCU, has been included in the sequence diagram to illustrate that the Media FSR Application Entity must execute the Display Directory activity before the Storage SCU may initiate a Transfer of SOP Instances activity.

The Read Media activity should always be preceded by a Display Directory activity.

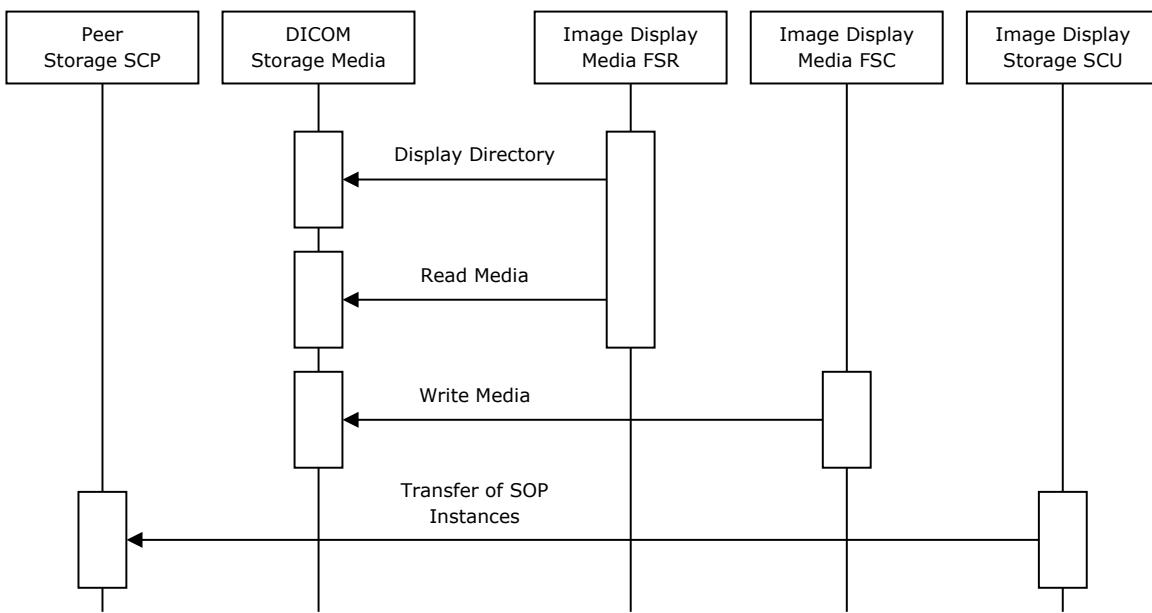


Figure 7: Sequencing of Real World Activities.

5.1.4 File Meta Information for Implementation Class and Version

The File Meta Information for the Implementation Class and Version is listed in Table 31.

| | |
|-----------------------------|------------------------------|
| Implementation Class UID | 1.3.6.1.4.1.16978.0.3.5.4.31 |
| Implementation Version Name | EV-3.5.4-31 |

Table 31: File Meta Information for Implementation Class and Version.

5.2 AE Specifications

5.2.1 AE Specification: Media FSR

The related application profiles, real world activities, and roles for the Media FSR Application Entity are listed in Table 32.

| Supported Application Profile | Real World Activity | Roles | SC Option |
|--|---------------------|-------|-------------|
| General Purpose CD-R Interchange | Display Directory | FSR | Interchange |
| | Read Media | FSR | Interchange |
| General Purpose Interchange on DVD-RAM Media | Display Directory | FSR | Interchange |
| | Read Media | FSR | Interchange |

Table 32: Media FSR: Related Application Profiles, Real World Activities, and Roles.

5.2.1.1 File Meta Information: Media FSR

The Media FSR Application Entity creates no File Meta Information.

5.2.1.2 Real-World Activities

5.2.1.2.1 Activity: Display Directory

5.2.1.2.1.1 Description and Sequencing of Activities

The local user at the Image Display inserts a CD-R/RW, a DVD-R/RW, a DVD+R/RW, or a DVD-RAM media into the media device, and invokes “Open CD-ROM/DVD” from the EasyViz Workflow Manager. The Media FSR Application Entity will then read the media directory, and display a list of stored DICOM Instances in the Workflow Manager.

5.2.1.2.1.2 Media Storage Application Profile

The Media Storage Application Profile for the Display Directory activity supports the Abstract Syntaxes and Transfer Syntaxes listed in Table 33.

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|--------------------------------|---|---|------|-------------|
| Name | UID | Name List | UID List | | |
| Basic Directory | 1.2.840.10008.1.3.10 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Computed Radiography Image Storage | 1.2.840.10008.5.1.4.1.1.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| CT Image Storage | 1.2.840.10008.5.1.4.1.1.2 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Digital Mammography X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.2 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Digital Mammography X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.2.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Breast Tomosynthesis Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.13.1.3 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Digital X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Digital X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Hardcopy Grayscale Image Storage SOP Class | 1.2.840.10008.5.1.1.29 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| MR Image Storage | 1.2.840.10008.5.1.4.1.1.4 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Ultrasound Image Storage | 1.2.840.10008.5.1.4.1.1.6.1 | Implicit VR LittleEndian Explicit VR LittleEndian Explicit VR BigEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Ultrasound Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.6 | Implicit VR LittleEndian Explicit VR LittleEndian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 | FSR | Interchange |

| | | | | | |
|---------------------------------------|------------------------------|--|---|-----|-------------|
| | | Explicit VR Big Endian | 1.2.840.10008.1.2.2 | | |
| X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| X-Ray Radiofluoroscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |

Table 33: Media FSR: Media Storage Application Profile for the Read Directory activity.

5.2.1.2.2 Activity: Read Media

5.2.1.2.2.1 Description and Sequencing of Activities

Having listed the contents of the storage media using the Display Directory activity, the user may read one or more of the stored DICOM Instance using the appropriate EasyViz CAM. Note that the stored DICOM Instances are not imported to the local database. If the user wishes to import the store DICOM Instances this may be done using the Transfer Instances activity of the Storage SCU Application Entity, see section 3.1.5.

5.2.1.2.2.2 Media Storage Application Profile

The Media Storage Application Profile for the Read Media activity supports the Abstract Syntaxes and Transfer Syntaxes listed in Table 34.

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|--------------------------------|--|---|------|-------------|
| Name | UID | Name List | UID List | | |
| Computed Radiography Image Storage | 1.2.840.10008.5.1.4.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| CT Image Storage | 1.2.840.10008.5.1.4.1.1.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Digital Mammography X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Digital Mammography X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.2.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Breast Tomosynthesis Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.13.1.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Digital X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Digital X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Hardcopy Grayscale Image Storage SOP Class | 1.2.840.10008.5.1.1.29 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| MR Image Storage | 1.2.840.10008.5.1.4.1.1.4 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |

| | | | | | |
|---------------------------------------|------------------------------|--|---|-----|-------------|
| Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Ultrasound Image Storage | 1.2.840.10008.5.1.4.1.1.6.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| Ultrasound Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.6 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| X-Ray Radiofluoroscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |

Table 34: Media FSR: Media Storage Application Profile for the Read Media activity.

5.2.2 AE Specification: Media FSC

The related application profiles, real world activities, and roles for the Media FSC Application Entity are listed in Table 35.

| Supported Application Profile | Real World Activity | Roles | SC Option |
|--|---------------------|-------|-------------|
| General Purpose CD-R Interchange | Write Media | FSC | Interchange |
| General Purpose Interchange on DVD-RAM Media | Write Media | FSC | Interchange |

Table 35: Media FSC: Related Application Profiles, Real World Activities, and Roles.

5.2.2.1 File Meta Information: Media FSC

Although the Media FSC creates DICOM File Meta Information for each file that it stores, it does not store information, which is specific to the Media FSC Application Entity. In particular, the Media FSC does not set the Source Application Entity Title.

5.2.2.2 Real-World Activities

5.2.2.2.1 Activity: Write Media

5.2.2.2.1.1 Description and Sequencing of Activity

The local user at the Image Display inserts a CD-R/RW, a DVD-R/RW, a DVD+R/RW, or a DVD-RAM media into the media device, selects a number of DICOM Instances in the Workflow Manager, and invokes “Export”. The Media FSC Application Entity will then create the file set corresponding to the selected DICOM Instances.

Note that it is possible to export to a non-local media device.

5.2.2.2.1.2 Media Storage Application Profile

The Media Storage Application Profile for the Write Media activity supports the Abstract Syntaxes and Transfer Syntaxes listed in Table 36.

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|-----------------|----------------------|--|---|------|-------------|
| Name | UID | Name List | UID List | | |
| Basic Directory | 1.2.840.10008.1.3.10 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |

| Abstract Syntax | | Transfer Syntax | | Role | Ext. Neg |
|--|--------------------------------|--|---|------|-------------|
| Name | UID | Name List | UID List | | |
| Computed Radiography Image Storage | 1.2.840.10008.5.1.4.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| CT Image Storage | 1.2.840.10008.5.1.4.1.1.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| Digital Mammography X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| Digital Mammography X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.2.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| Breast Tomosynthesis Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.13.1.3 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| Digital X-Ray Image Storage – For Presentation | 1.2.840.10008.5.1.4.1.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| Digital X-Ray Image Storage – For Processing | 1.2.840.10008.5.1.4.1.1.1.1.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| Hardcopy Grayscale Image Storage SOP Class | 1.2.840.10008.5.1.1.29 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSR | Interchange |
| MR Image Storage | 1.2.840.10008.5.1.4.1.1.4 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| Ultrasound Image Storage | 1.2.840.10008.5.1.4.1.1.6.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| Ultrasound Image Storage (Retired) | 1.2.840.10008.5.1.4.1.1.6 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| X-Ray Angiographic Image Storage | 1.2.840.10008.5.1.4.1.1.12.1 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |
| X-Ray Radiofluoroscopic Image Storage | 1.2.840.10008.5.1.4.1.1.12.2 | Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian | 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 | FSC | Interchange |

Table 36: Media FSR: Media Storage Application Profile for the Write Media activity.

5.3 Augmented and Private Application Profiles

The EasyViz Image Display does not support any Augmented or Private Application Profiles.

5.4 Media Configuration

The EasyViz Image Display does not depend on media configuration at installation time.

6. Support of Character Sets

6.1 Overview

EasyViz Image Display supports the default character repertoire. Support extends to correctly decoding and displaying the correct symbol for all names and strings received over the network, found in the DICOMDIR, or found in the local database.

No specific support for sorting of strings other than in the default character set is provided by the EasyViz Image Display.

6.2 Character Sets

EasyViz supports the extended character sets listed in Table 37.

| Character Set Description | Defined Term |
|---------------------------|--------------|
| Latin 1 | ISO_IR 100 |
| ASCII | ISO_IR 6 |
| Latin 2 | ISO_IR 101 |
| Latin 3 | ISO_IR 109 |
| Latin 4 | ISO_IR 110 |
| Cyrillic | ISO_IR 144 |
| Arabic | ISO_IR 127 |
| Greek | ISO_IR 126 |
| Hebrew | ISO_IR 138 |
| Latin 5 | ISO_IR 148 |
| UTF-8 | ISO_IR 192 |

Table 37: Supported specific character set defined terms.

6.3 Character Set Configuration

Whether or not characters are displayed correctly depends on the presence of font support in the underlying operating system.

It may be necessary for the user to add one of the “all Unicode” fonts to their system configuration in order to correctly display characters that would not typically be used in the default locale. Note, that the font installation should happen at the server side, if EasyViz Image Display is used in a telemedicine configuration.

7. Security

7.1 Security Profiles

The EasyViz Image Display does not support any DICOM security profiles.

7.2 Association Level Security

Neither the Query/Retrieve SCU, Storage SCU, nor the Print Management SCU Application Entities accepts Association Requests.

The Storage SCP accepts all association requests, i.e. it is not possible to restrict associations based on Calling AET. The Storage SCP only verifies that it has been called with the correct AET.

7.3 Application Level Security

The EasyViz Image Display applications can be configured to use either MIT Kerberos or the internal database for user authentication. It is not possible to configure the EasyViz Image Display not to require user authentication. By default, the internal database is used.

When using MIT Kerberos for user authentication, it is possible to integrate the EasyViz Image Display with Microsoft Active Directory. This allows Microsoft Windows users to use their regular username and password to access the EasyViz Image Display.

8. Annexes

8.1 IOD Contents

8.1.1 Created SOP Instance(s)

The EasyViz Image Display creates Key Objects and Grayscale Softcopy Presentation States. Attributes of Key Objects created by EasyViz Image Display can be seen in Table 38. Attributes of the Grayscale Softcopy Presentation State can be seen in Table 39.

The follow tables use a number of abbreviations. The abbreviations used in the "Presence of ..." column are:

| | |
|--------|------------------------------|
| VNAP | Value not always present |
| ANAP | Attribute not always present |
| ALWAYS | Always present |
| EMPTY | Attribute sent without value |

The abbreviations used in the "Source" column are:

| | |
|--------|---|
| IMAGE | Attribute value source is referenced image |
| USER | Attribute value source is user input |
| AUTO | Attribute value is auto generated |
| CONFIG | Attribute value source is a configuration parameter |

8.1.1.1 Key Object Selection Document IOD

| IE | Module | Reference | Presence of Module |
|-----------|----------------------------|-----------|--------------------|
| Patient | Patient | Table 40 | ALWAYS |
| Study | General Study | Table 41 | ALWAYS |
| | Patient Study | | EMPTY |
| Series | Key Object Document Series | Table 44 | ALWAYS |
| Equipment | General Equipment | Table 43 | ALWAYS |
| Document | Key Object Document | Table 45 | ALWAYS |
| | SR Document Content | Table 46 | ALWAYS |
| | SOP Common | Table 47 | ALWAYS |

Table 38: IOD of Created Key Object Selection Document SOP Instances.

Attributes of Key Objects created by EasyViz Image Display can be seen in section 7.1.1.3 and section 7.1.1.4.

8.1.1.2 Grayscale Softcopy Presentation State IOD

| IE | Module | Reference | Presence of Module |
|--------------------|-----------------------------------|-----------|--|
| Patient | Patient | Table 40 | ALWAYS |
| Study | General Study | Table 41 | ALWAYS |
| | Presentation Series | | EMPTY |
| Series | Key Object Document Series | Table 48 | ALWAYS |
| Equipment | General Equipment | Table 43 | ALWAYS |
| Presentation State | Presentation State Identification | Table 49 | ALWAYS |
| | Presentation State Relationship | Table 50 | ALWAYS |
| | Display Shutter | | EMPTY |
| | Displayed Area | Table 51 | ALWAYS |
| | Graphic Annotation | Table 52 | USER |
| | Spatial Transformation | Table 53 | ALWAYS |
| | Graphic Layer | Table 54 | USER |
| | Modality LUT | Table 55 | ANAP – If source image contains Modality transformation, this module is created. |
| | Softcopy VOI LUT | Table 56 | ALWAYS |
| | Softcopy Presentation LUT | Table 57 | ALWAYS |
| | SOP Common | Table 58 | ALWAYS |

Table 39: IOD of Created Grayscale Softcopy Presentation State SOP Instances.

Attributes of Grayscale Softcopy Presentation States created by EasyViz Image Display can be seen in section 7.1.1.3 and section 7.1.1.5.

8.1.1.3 Common Modules

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|----------------------|--------------|----|------------------------|-------------------|--------|
| Patient's Name | (0010, 0010) | PN | From referenced image. | ALWAYS | IMAGE |
| Patient ID | (0010, 0020) | LO | From referenced image. | ALWAYS | IMAGE |
| Issuer of Patient ID | (0010, 0021) | LO | From referenced image. | ALWAYS | IMAGE |
| Patient's Birth Date | (0010, 0030) | DA | From referenced image. | ALWAYS | IMAGE |
| Patient's Sex | (0010, 0040) | CS | From referenced image. | ALWAYS | IMAGE |
| Patient's Birth Time | (0010, 0032) | TM | From referenced image. | ALWAYS | IMAGE |

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|---------------------|--------------|----|------------------------|-------------------|--------|
| Other Patient IDs | (0010, 1000) | LO | From referenced image. | ALWAYS | IMAGE |
| Other Patient Names | (0010, 1001) | PN | From referenced image. | ALWAYS | IMAGE |
| Ethnic Group | (0010, 2160) | SH | From referenced image. | ALWAYS | IMAGE |
| Patient Comments | (0010, 4000) | LT | From referenced image. | ALWAYS | IMAGE |

Table 40: Patient Module of Created SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|----------------------------|--------------|----|--|-------------------|--------|
| Study Instance UID | (0020, 000D) | UI | From referenced image. | ALWAYS | IMAGE |
| Study Date | (0008, 0020) | DA | From referenced image. | ALWAYS | IMAGE |
| Study Time | (0008, 0030) | TM | From referenced image. | ALWAYS | IMAGE |
| Referring Physician's Name | (0008, 0090) | PN | From referenced image. | ALWAYS | IMAGE |
| Study ID | (0020, 0010) | SH | From referenced image, or "NoValue" if no value specified by referenced image. | ALWAYS | IMAGE |
| Accession Number | (0008, 0050) | SH | From referenced image. | ALWAYS | IMAGE |
| Study Description | (0008, 1030) | LO | From referenced image. | ALWAYS | IMAGE |

Table 41: General Study Module of Created SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|---------------------|--------------|----|-------------------------------|-------------------|--------|
| Modality | (0008, 0060) | CS | Auto-generated: "KO" or "PR". | ALWAYS | AUTO |
| Series Instance UID | (0020, 000E) | UI | Auto-generated. | ALWAYS | AUTO |
| Series Number | (0020, 0011) | IS | Auto-generated. | ALWAYS | AUTO |
| Series Date | (0008, 0021) | DA | Auto-generated: Current date. | ALWAYS | AUTO |
| Series Time | (0008, 0031) | TM | Auto-generated: Current time. | ALWAYS | AUTO |
| Series Description | (0008, 103E) | LO | From user input. | ALWAYS | USER |

Table 42: General Series Module of Created SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|------------------|--------------|----|----------------------------|-------------------|--------|
| Manufacturer | (0008, 0070) | LO | From system configuration. | ALWAYS | CONFIG |
| Software Version | (0018, 1020) | LO | From system configuration. | ALWAYS | CONFIG |

Table 43: General Equipment Module of Created SOP Instances.

8.1.1.4 Key Object Selection Document Modules

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|---------------------|--------------|----|-----------------|-------------------|--------|
| Modality | (0008, 0060) | CS | KO | ALWAYS | AUTO |
| Series Instance UID | (0020, 000E) | UI | Auto-generated. | ALWAYS | AUTO |
| Series Number | (0020, 0011) | IS | Auto-generated. | ALWAYS | AUTO |

Table 44: Key Object Document Series Module of Created KO SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|---|--------------|-----|------------------------|-------------------|--------|
| Instance Number | (0020, 0013) | IS | Auto-generated. | ALWAYS | AUTO |
| Content Date | (0008, 0023) | DA | Auto-generated. | ALWAYS | AUTO |
| Content Time | (0008, 0033) | TM | Auto-generated. | ALWAYS | AUTO |
| Current Requested Procedure Evidence Sequence | (0040, A375) | | One or more items. | ALWAYS | AUTO |
| >Study Instance UID | (0020, 000D) | UI | From referenced image. | ALWAYS | AUTO |
| >Referenced Series Sequence | (0008, 1115) | SQ | One or more items. | ALWAYS | AUTO |
| >Series Instance UID | (0020, 000E) | UI | From referenced image. | ALWAYS | AUTO |
| >Referenced SOP Sequence | (0008, 1199) | SQ | One or more items. | ALWAYS | AUTO |
| >>Referenced SOP Class UID | (0008, 1150) | UI | From referenced image. | ALWAYS | AUTO |
| >>Referenced SOP Instance UID | (0008, 1155) | UID | From referenced image. | ALWAYS | AUTO |

Table 45: Key Object Document Module of Created KO SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|----------------------------|--------------|----|--|-------------------|--------|
| Value Type | (0040, A040) | CS | "CONTAINER" | ALWAYS | AUTO |
| Concept Name Code Sequence | (0040, A043) | SQ | Sequence containing one item. | ALWAYS | AUTO |
| >Code Value | (0008, 0100) | SH | User input – but restricted to: 113000-113012, or 113026. | ALWAYS | USER |
| >Coding Scheme | (0008, 0102) | SH | "DCM" | ALWAYS | AUTO |
| >Code Meaning | (0008, 0104) | LO | User input – but restricted to: "Of Interest", "Rejected for Quality Reasons", "For Referring Provider", "For Surgery", "For Teaching", "For Conference", "For | ALWAYS | USER |

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|----------------|--------------|----|--|-------------------|--------|
| | | | Therapy", "For Patient", "For Peer Review", "For Research", "Quality Issue", "Document Title Modifier", "Key Object Description", "Double exposure". | | |
| Text Value | (0040, A160) | | User input. | ALWAYS | USER |

Table 46: SR Document Content Module of Created KO SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|------------------------|--------------|----|-------------------------------|-------------------|--------|
| Specific Character Set | (0008, 0005) | CS | "ISO_IR 100" | ALWAYS | AUTO |
| SOP Class UID | (0008, 0016) | UI | 1.2.840.10008.5.1.4.1.1.88.59 | ALWAYS | AUTO |
| SOP Instance UID | (0008, 0018) | UI | Auto-generated. | ALWAYS | AUTO |

Table 47: SOP Common of Created KO SOP Instances.

8.1.1.5 Grayscale Softcopy Presentation State Modules

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|----------------|--------------|----|-------|-------------------|--------|
| Modality | (0008, 0060) | CS | PR | ALWAYS | AUTO |

Table 48: Presentation Series Module of Created GSPS SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|----------------------------|--------------|----|------------------------------------|-------------------|--------|
| Instance Number | (0020, 0013) | IS | Auto-generated. | ALWAYS | AUTO |
| Presentation Label | (0070, 0080) | CS | From user input. | ALWAYS | USER |
| Presentation Description | (0070, 0081) | LO | From user input. | ALWAYS | USER |
| Presentation Creation Date | (0070, 0082) | DA | Auto-generated: Current date. | ALWAYS | AUTO |
| Presentation Creation Time | (0070, 0083) | TM | Auto-generated: Current time. | ALWAYS | AUTO |
| Content Creator's Name | (0070, 0084) | PN | Auto-generated: User display name. | ALWAYS | AUTO |

Table 49: Presentation State Identification Module of Created GSPS SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|----------------------------|--------------|----|------------------------|-------------------|--------|
| Referenced Series Sequence | (0008, 1115) | SQ | One or more items. | ALWAYS | AUTO |
| >Series Instance UID | (0020, 000E) | UI | From referenced image. | ALWAYS | AUTO |
| >Referenced Image Sequence | (0008, 1140) | SQ | From referenced image. | ALWAYS | AUTO |

| | | | | | |
|-------------------------------|--------------|----|---|--------|------|
| >>Referenced SOP Class UID | (0008, 1150) | UI | From referenced image. | ALWAYS | AUTO |
| >>Referenced SOP Instance UID | (0008, 1155) | UI | From referenced image. | ALWAYS | AUTO |
| >>Referenced Frame Number | (0008, 1160) | IS | If referenced image is a multi-frame image. | ANAP | AUTO |

Table 50: Presentation State Relationship Module of Created GSPS SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|--|--------------|----|---|-------------------|--------|
| Displayed Area Selection Sequence | (0070, 005A) | SQ | One or more items. | ALWAYS | AUTO |
| >Referenced Image Sequence | (0008, 1140) | SQ | One or more items. | ALWAYS | AUTO |
| >>Referenced SOP Class UID | (0008, 1150) | UI | From referenced image. | ALWAYS | AUTO |
| >>Referenced SOP Instance UID | (0008, 1155) | UI | From referenced image. | ALWAYS | AUTO |
| >>Referenced Frame Number | (0008, 1160) | IS | If referenced image is a multi-frame image. | ANAP | AUTO |
| >Displayed Area Top Left Hand Corner | (0070, 0052) | SL | From current display settings. | ALWAYS | AUTO |
| >Displayed Area Bottom Right Hand Corner | (0070, 0053) | SL | From current display settings. | ALWAYS | AUTO |
| >Presentation Size Mode | (0070, 0100) | CS | From current display settings. | ALWAYS | AUTO |
| >Presentation Pixel Spacing | (0070, 0101) | DS | From current display settings. | ANAP | AUTO |
| >Presentation Pixel Aspect Ratio | (0070, 0102) | IS | From referenced image. | ANAP | IMAGE |
| >Presentation Pixel Magnification Ratio | (0070, 0103) | FL | From referenced image. | ANAP | IMAGE |

Table 51: Displayed Area Module of Created GSPS SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|-------------------------------|--------------|----|------------------------|-------------------|--------|
| Graphic Annotation Sequence | (0070, 0001) | SQ | Zero or more items | ANAP | AUTO |
| >Referenced Image Sequence | (0008, 1140) | SQ | One or more items. | ALWAYS | AUTO |
| >>Referenced SOP Class UID | (0008, 1150) | UI | From referenced image. | ALWAYS | AUTO |
| >>Referenced SOP Instance UID | (0008, 1155) | UI | From referenced image. | ALWAYS | AUTO |

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|--|--------------|----|---|-------------------|--------|
| >>Referenced Frame Number | (0008, 1160) | IS | If referenced image is a multi-frame image. | ANAP | AUTO |
| >Graphic Layer | (0070, 0002) | CS | Layer in Graphic Layer Module. | ALWAYS | AUTO |
| >Text Object Sequence | (0070, 0008) | SQ | One or more items if text annotations are present. | ANAP | AUTO |
| >>Bounding Box Annotation Units | (0070, 0003) | CS | "PIXEL" | ALWAYS | AUTO |
| >>Anchor Point Annotation Units | (0070, 0004) | CS | "PIXEL" | ALWAYS | AUTO |
| >>Unformatted Text Value | (0070, 0006) | ST | From user input. | ALWAYS | USER |
| >>Bounding Box Top Left Hand Corner | (0070, 0010) | FL | From current display settings | ALWAYS | AUTO |
| >>Bounding Box Bottom Right Hand Corner | (0070, 0011) | FL | From current display settings | ALWAYS | AUTO |
| >>Bounding Box Text Horizontal Justification | (0070, 0012) | CS | From user input | ALWAYS | USER |
| >>Anchor Point | (0070, 0014) | FL | From user input. | ALWAYS | USER |
| >>Anchor Point Visibility | (0070, 0015) | CS | From user input. | ALWAYS | USER |
| >Graphic Object Sequence | (0070, 0009) | SQ | One or more items if graphic annotations are present. | ANAP | AUTO |
| >>Graphic Annotation Units | (0070, 0005) | CS | "PIXEL" | ALWAYS | AUTO |
| >>Graphic Dimensions | (0070, 0020) | US | 2 | ALWAYS | AUTO |
| >>Number of Graphic Points | (0070, 0021) | US | From user input. | ALWAYS | USER |
| >>Graphic Data | (0070, 0022) | FL | From user input. | ALWAYS | USER |
| >>Graphic Type | (0070, 0023) | CS | One of: "POINT", "POLYLINE", "INTERPOLATED", "CIRCLE" or "ELLIPSE". | ALWAYS | USER |
| >>Graphic Filled | (0070, 0024) | CS | From user input. | ALWAYS | USER |

Table 52: Graphic Annotation Module of Created GSPS SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|-----------------------|--------------|----|--------------------------------|-------------------|--------|
| Image Rotation | (0070, 0042) | US | From current display settings. | ALWAYS | AUTO |
| Image Horizontal Flip | (0070, 0041) | CS | From current display settings. | ALWAYS | AUTO |

Table 53: Spatial Transformation Module of Created GSPS SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|------------------------|--------------|----|-------------------------------|-------------------|--------|
| Graphic Layer Sequence | (0070, 0060) | SQ | One or more items | ALWAYS | AUTO |
| >Graphic Layer | (0070, 0002) | CS | LAYER1, LAYER2, ... | ALWAYS | AUTO |
| >Graphic Layer Order | (0070, 0062) | IS | From current display settings | ALWAYS | AUTO |

Table 54: Graphic Layer Module of Created GSPS SOP Instances.

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|-----------------------|--------------|----|--|-------------------|--------|
| Modality LUT Sequence | (0028, 3000) | SQ | Zero or one item. Either the Modality LUT Sequence is present with one item, or the Rescale Intercept/Slope/Type is present. | ANAP | AUTO |
| >LUT Descriptor | (0028, 3002) | US | From referenced image. | ALWAYS | AUTO |
| >Modality LUT Type | (0028, 3004) | LO | From referenced image. | ALWAYS | AUTO |
| >LUT Data | (0028, 3006) | US | LUT | ALWAYS | AUTO |
| Rescale Intercept | (0028, 1052) | DS | From referenced image. If referenced image does not contain rescale intercept, this value is set to 0.0. | ANAP | AUTO |
| Rescale Slope | (0028, 1053) | DS | From referenced imaged. If referenced image does not contain rescale slope, this value is set to 1.0. | ANAP | AUTO |
| Rescale Type | (0028, 1054) | LO | "US" | ANAP | AUTO |

Table 55: Modality LUT Module of Created GSPS SOP Instances

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|-------------------------------|--------------|----|---|-------------------|--------|
| Softcopy VOI LUT Sequence | (0028, 3110) | SQ | One or more items. | ALWAYS | AUTO |
| >Referenced Image Sequence | (0008, 1140) | SQ | One or more items. | ALWAYS | AUTO |
| >>Referenced SOP Class UID | (0008, 1150) | UI | From referenced image. | ALWAYS | AUTO |
| >>Referenced SOP Instance UID | (0008, 1155) | UI | From referenced image. | ALWAYS | AUTO |
| >>Referenced Frame Number | (0008, 1160) | IS | If referenced image is a multi-frame image. | ANAP | AUTO |
| >Window Center | (0028, 1050) | DS | From current display settings. | ALWAYS | AUTO |
| >Window Width | (0028, 1051) | DS | From current display settings. | ALWAYS | AUTO |

| | | | | | |
|------------------------------------|--------------|----|-----------------------|------|------|
| >Window Center & Width Explanation | (0028, 1055) | LO | Name of Window Preset | ANAP | AUTO |
|------------------------------------|--------------|----|-----------------------|------|------|

Table 56: Softcopy VOI LUT Module of Created GSPS SOP Instances

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|------------------------|--------------|----|--|-------------------|--------|
| Presentation LUT Shape | (2050, 0020) | CS | Auto-generated: "IDENTITY" or "INVERSE". | ALWAYS | AUTO |

Table 57: Softcopy Presentation LUT Module of Created GSPS SOP Instances

| Attribute Name | Tag | VR | Value | Presence of Value | Source |
|------------------------|--------------|----|------------------------------|-------------------|--------|
| Specific Character Set | (0008, 0005) | CS | "ISO_IR 100" | ALWAYS | AUTO |
| SOP Class UID | (0008, 0016) | UI | 1.2.840.10008.5.1.4.1.1.11.1 | ALWAYS | AUTO |
| SOP Instance UID | (0008, 0018) | UI | Auto-generated. | ALWAYS | AUTO |

Table 58: SOP Common Module of Created GSPS SOP Instances

8.1.2 Usage of Attributes of Received IOD's

The local database and remote query make use of conventional identification attributes to distinguish patients, studies, series and instances. In particular, if two patients have the same value for Patient ID, the EasyViz Image Display will treat them as the same patient.

8.1.3 Attribute Mapping

Not applicable.

8.1.4 Coerced/Modified Fields

The EasyViz Image Display does not perform any coercion.

8.2 Data Dictionary of Private Attributes

The EasyViz Image Display does not define any private attributes.

8.3 Coded Terminology and Templates

The value for Coded Meaning will be displayed for all coded values. The EasyViz Image Display does not provide a local lexicon to lookup alternative code meanings.

8.4 Grayscale Image Consistency

The image display monitor attached to EasyViz can – if supported by the monitor – be calibrated according to the DICOM Grayscale Standard Display Function (GSDF). The monitors Service/Installation Tool are used together with a luminance meter to measure the Characteristics Curve for the display system and the current ambient light. See the product Service Manual for details on the calibration procedure and supported calibration hardware. The result of the calibration procedure is a Monitor Correction LUT that will be active within the display system after a system reboot.

8.5 Standard Extended/Specialized/Private SOP Classes

8.5.1 MI 3D Softcopy Presentation State Private SOP Class

The General 3D CAM generates 3D Softcopy Presentation States in a private SOP Class

SOP Class (private): MI 3D Softcopy Presentation State

SOP Class UID: 1.3.6.1.4.1.16978.3.1

8.6 Private Transfer Syntaxes

The EasyViz Image Display does not support any private transfer syntaxes.